

# BIOSCIENCE INTERNATIONAL

Innovative Microbiology Products  
 11333 Woodglen Drive • Rockville, Maryland 20852  
 301.231.7400 • www.biosci-intl.com • fax: 301.231.7277

## CERTIFICATE OF CALIBRATION

Model:	SAS Super 100
Air Sampler Serial #:	00-C-01686
Air Sampler Head Serial #:	15901
Customer:	Aerobiology Laboratory
Customer Asset ID #:	n/a
Calibration performed at:	JBW site 10242 Little Rock Ln Frederick, MD 21702


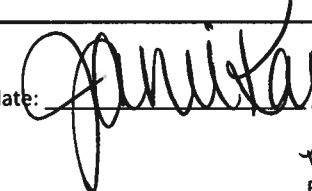
Cal. Date:	28 Mar 2020
Cal. Due:	28 Mar 2021 (12 months)
Procedure:	EOP-030
Certificate #:	00-C-01686-1918
Volume sampled (L):	1000
Calibrated w/media type:	BBL TSA Petri
Plate Lot #:	9317765
Plate Exp Date:	4/27/2020

	As Found	In Tolerance	As Left	In Tolerance	Acceptable Range
Battery output (Volts):	9.9	n/a	9.6	n/a	>8.2
Temperature (F°):	70.3	n/a	70.3	n/a	59 - 95
Barometric pressure (in. HG):	30.2	n/a	30.2	n/a	n/a
Time to sample 1000 Liters (min)	9.85	n/a	9.85	n/a	n/a
Temp. & Pressure Standardization Factor:	1.01	n/a	1.01	n/a	n/a
Air velocity reading (ft/min)	56.0	n/a	56.0	n/a	n/a
Air velocity reading (m/sec)	0.284	n/a	0.284	n/a	n/a
Standardized air velocity reading (m/sec)	0.287	n/a	0.287	n/a	n/a
Standardized Air Flow (L/min)	101.5	Yes	101.5	Yes	95 - 105

Additional heads inspected and determined to be within +/-2%:	n/a
Additional service, preventative maintenance, or calibration notes:	n/a

*Bioscience International certifies that the above described instrument conforms to the original manufacturer's tolerances for the parameters listed (not applicable to As Found data) & has been calibrated in accordance with ISO 17025:2017 guidelines using standards whose accuracies are traceable to the U.S. National Institute of Standards and Technology (NIST) or have been verified with respect to instrumentation whose accuracy is traceable to NIST, or is derived from accepted values of physical constants. Instruments are calibrated with a test uncertainty ratio of 4:1 or greater whenever possible, with uncertainty defined as within a 95 % confidence interval using a coverage factor of k = 2. In all cases, statistical methods are used to minimize uncertainty using the best commercially available methods. Calibration results relate only to the items listed above; in particular, the instrument should be recalibrated prior to switching to a different media size (e.g., from 90mm petri dishes to 55mm contact plates or vice versa).*

<u>Measurement Standards</u>			
ID	Description	Last Cal.	Cal. Due
J-T95452002007	Velocity	1/10/2020	1/9/2021
J-6530-181788940	Temperature & Pressure	12/7/2018	12/7/2020

Work performed by / date:  / 3-18-20 Reviewed by / date:  3-28-20

Document #200  
Page 1 of 1

Version 2.2  
Effective 6/17/2019